

Instrument calibration sheet

Certificate N°	000149	Date of issue	17/10/2019
Client	ENEL Produzione	Work order	8000000591

Instrument specification

Type	pH meter	Manufacturer	Endress-Hauser	Max capacity	14
Model	Liquiline CM442	Serial number	E3087105G00	Readability	0,1
Description	C1 Itar pH meter			Unit of measure	pH

Test ambient conditions

Location	ENEL - C1 Itar		Date of test	10/09/2019	09:11
Temperature	23°C	Humidity	75%	Pressure	1021hPa

Standard certificates used

Name	Number	Issuer	Date of issue
pH	12105826	XS Solutions	21/05/2018

Calibration summary

Test	Certificate name	Uncertainty	Temperature	Humidity	Pressure
Repeatability	pH	0,053229pH	23°C	75%	1021hPa
Linearity	pH	0,080416pH	23°C	75%	1021hPa
Expanded uncertainty					0,160831pH

Notes

Technician
Provenza Luca


Repeatability

Measure	Nominal value	Conventional value	Read value	Deviation	Standard reference		
					Serial	Uncertainty	OIML
1	7	7	6,9	-0,1	51100143	0,01	
2	7	7	7	0	51100143	0,01	
3	7	7	6,9	-0,1	51100143	0,01	
4	7	7	6,9	-0,1	51100143	0,01	
5	7	7	6,9	-0,1	51100143	0,01	

Min value 6,9 Max value 7 Average value 6,92

Standard deviation (σ) 0,044721 Repeatability uncertainty 0,053229

Repeatability control chart

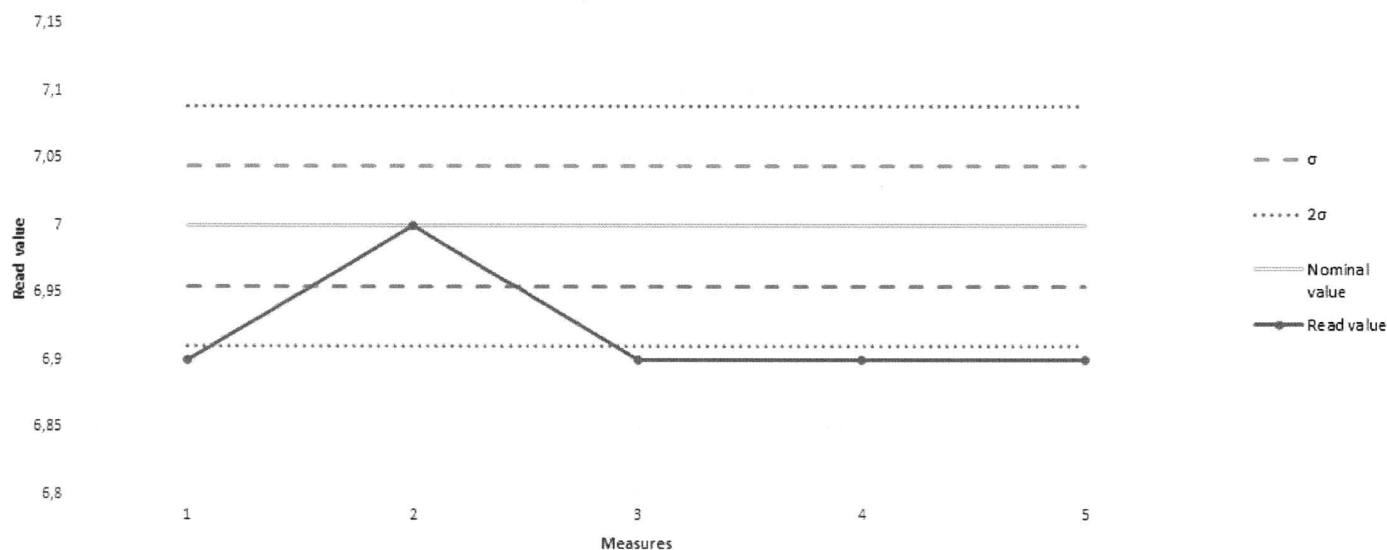

Technician
Provenza Luca


Linearity

Measure	Nominal value	Conventional value	Read value	Error	Uncertainty of error	Standard reference	
						Uncertainty	OIML
1	4,01	4,01	4	-0,01	0,077406	0,01	
2	7	7	7	0	0,077406	0,01	
3	10,01	10,01	9,9	-0,11	0,080416	0,02	

Min value 4 Max value 9,9 Average value 6,96667

Standard deviation 0,11 k-Factor: 2 (95,45%) Expanded uncertainty 0,160831

Linearity deviation

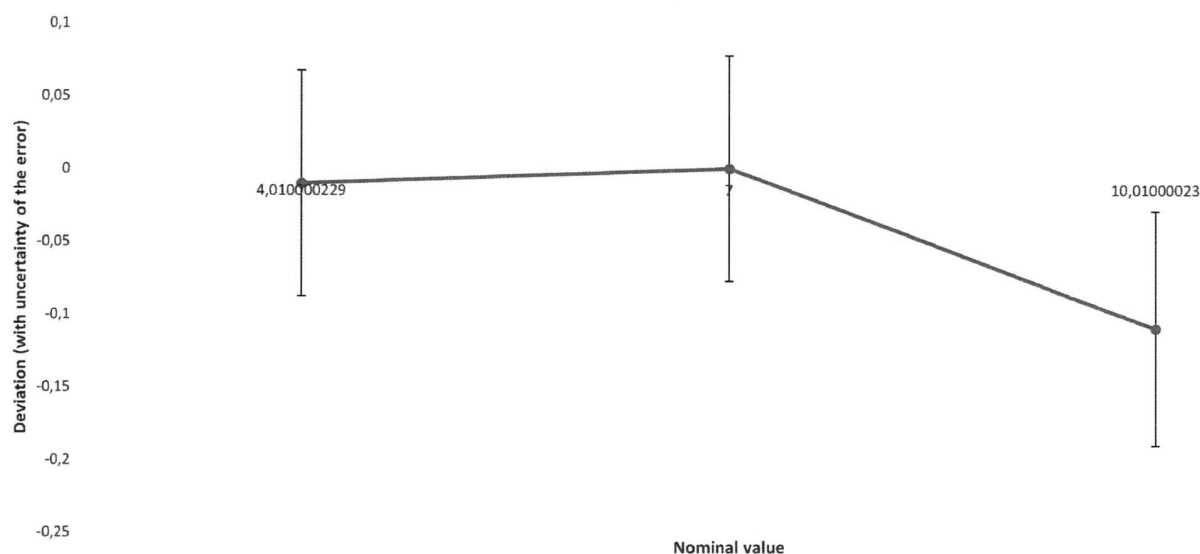

Technician
Provenza Luca

Formulas

Repeatability

The test consists in the repeated measure of the same reference value, under identical conditions of handling the reference and the instrument, and under constant test conditions, both as far as possible

Standard deviation is computed to allow an appraisal of the instrument's performance.

$$s(I) = \sqrt{\frac{1}{n-1} \sum_{i=1}^n (I_i - \bar{I})^2} \quad \bar{I} = \frac{1}{n} \sum_{i=1}^n I_i$$

Repeatability standard uncertainty has been computed with the following formula, taking into account instrument's scale interval (d)

$$u_{rep} = \sqrt{s(I)^2 + \left(\frac{d_I^2}{12}\right)}$$

Linearity

This test is performed with different test values distributed fairly evenly over the normal measuring range. The purpose of this test is an appraisal of the performance of the instrument over the whole measuring range.

The uncertainty of the error is computed with the following formula and takes into account repeatability and eccentricity uncertainty when applicable:

$$u(E) = \sqrt{u^2(I_{dig0}) + u^2(I_{dig1}) + u^2(I_{rep}) + u^2(I_{ecc}) + u^2(I_{mc}) + u^2(I_{mb}) + u^2(I_{md}) + u^2(I_{mconv})}$$

The terms relative to air buoyancy (mb) and convection effects (mconv) are considered negligible due to enough acclimatisation allowed to the instrument.

Expanded uncertainty has been computed with the following formula:

$$U = u(E)_{max} k$$

For this report a coverage factor of 2 as been considered giving an overall confidence level of 95,45%