

# Instrument calibration sheet

Certificate N°	000012/2021	Date of issue	21.06.21
Client	ENEL Produzione	Work order	8000000591

## Instrument specification

Type	pH meter	Manufacturer	Endress-Hauser	Serial number	E3087105G00
Min capacity	0	Max capacity	14	Model	Liquiline CM442
Readability At 0	0,1	Readability	0,1	Unit of measure	pH
Description	C1 Itar pH meter	Next Calibration	30.06.21		

## Test ambient conditions

Location	ENEL - C1 Itar			Date of test	21.06.21	00:00
Temperature	24,5°C	Humidity	69%	Pressure	1020hPa	

## Standard certificates used

Name	Number	Issuer	Date of issue
pH	17L93	Hanna Instruments	28.07.20

## Calibration summary

Test	Certificate name	Uncertainty	Temperature	Humidity	Pressure
Repeatability	pH	0,029212pH	28°C	71%	1020hPa
Linearity	pH	0,047958pH	16°C	70%	1018hPa

**Expanded uncertainty** **0,095917pH**

## Notes

Technician  
Provenza Luca


## Repeatability

Measure	Nominal value	Conventional value	Read value	Deviation	Standard reference		
					Serial	Uncertainty	OIML
1	7	7	7,01	0,01	06K92	0,01	
2	7	7	7,01	0,01	06K92	0,01	
3	7	7	7,02	0,02	06K92	0,01	
4	7	7	7,01	0,01	06K92	0,01	
5	7	7	7,01	0,01	06K92	0,01	

Min value 7,01 Max value 7,02 Average value 7,012

Standard deviation ( $\sigma$ ) 0,004472 Repeatability uncertainty 0,029212

Repeatability control chart

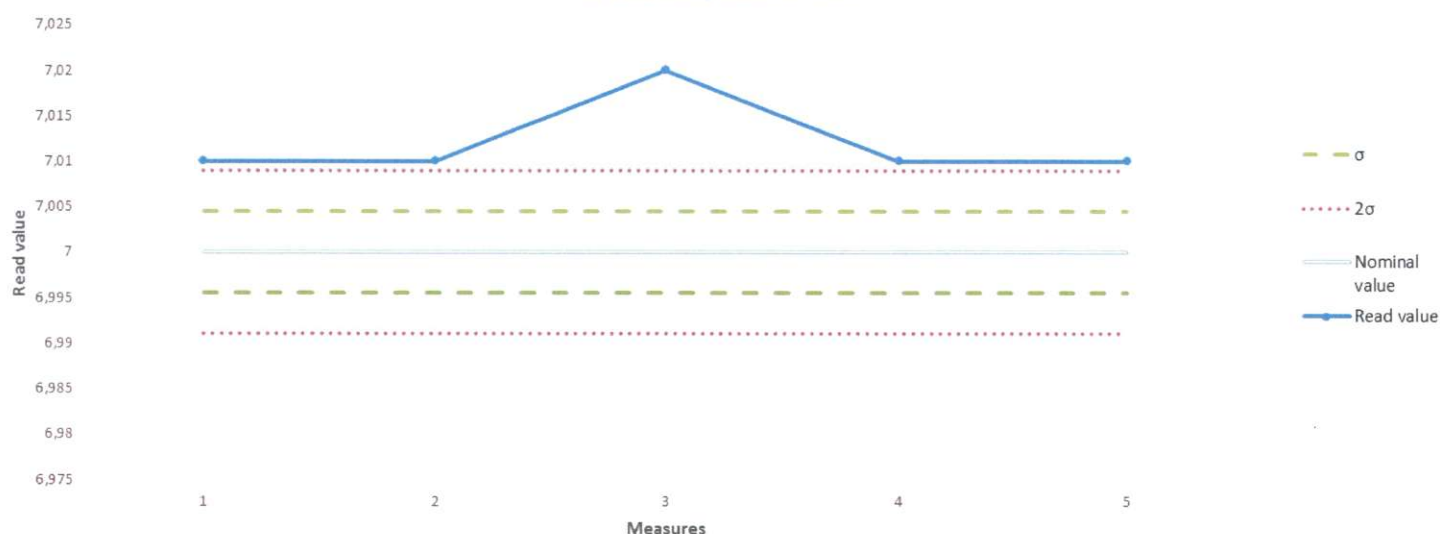

Technician  
Provenza Luca

## Linearity

Measure	Nominal value	Conventional value	Read value	Error	Uncertainty of error	Standard reference	
						Uncertainty	OIML
1	4,01	4,01	4,01	0	0,04272	0,01	
2	7,01	7,01	7,01	0	0,04272	0,01	
3	10,01	10,01	10,01	0	0,047958	0,02	

Min value 4,01

Max value 10,01

Average value

7,01


Standard deviation 0

k-Factor: 2 (95,45%)

Expanded uncertainty

0,095917

## Linearity deviation

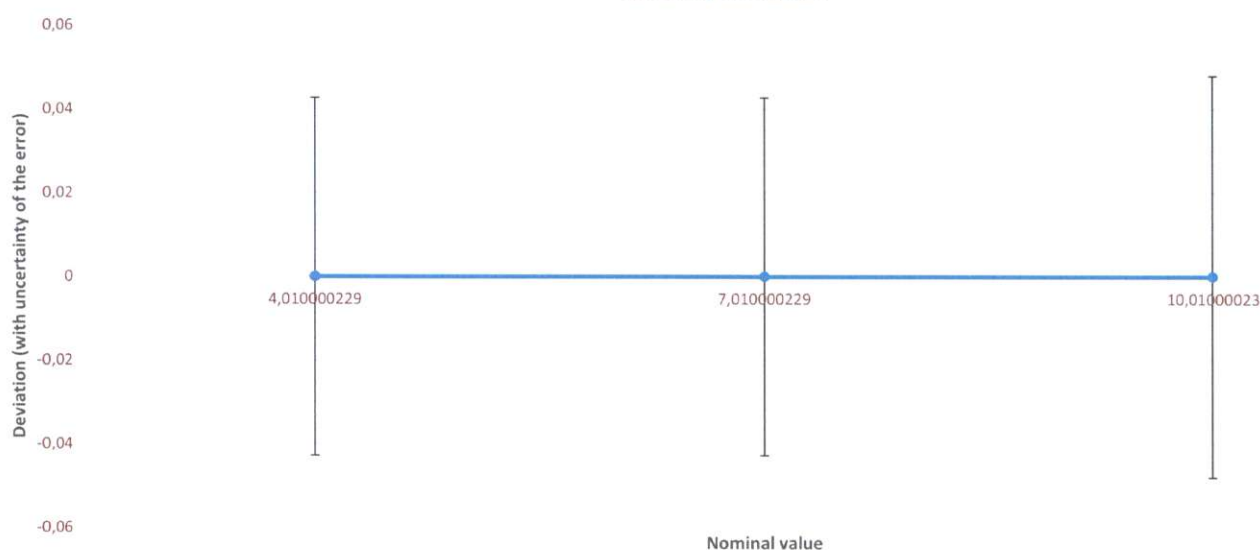

Technician  
Provenza Luca

## Formulas

### Repeatability

The test consists in the repeated measure of the same reference value, under identical conditions of handling the reference and the instrument, and under constant test conditions, both as far as possible

Standard deviation is computed to allow an appraisal of the instrument's performance.

$$s(I) = \sqrt{\frac{1}{n-1} \sum_{i=1}^n (I_i - \bar{I})^2} \quad \bar{I} = \frac{1}{n} \sum_{i=1}^n I_i$$

Repeatability standard uncertainty has been computed with the following formula, taking into account instrument's scale interval (d)

$$u_{rep} = \sqrt{s(I)^2 + \left(\frac{d_I^2}{12}\right)}$$

### Linearity

This test is performed with different test values distributed fairly evenly over the normal measuring range. The purpose of this test is an appraisal of the performance of the instrument over the whole measuring range.

The uncertainty of the error is computed with the following formula and takes into account repeatability and eccentricity uncertainty when applicable:

$$u(E) = \sqrt{u^2(I_{dig0}) + u^2(I_{dig1}) + u^2(I_{rep}) + u^2(I_{ecc}) + u^2(I_{mc}) + u^2(I_{mb}) + u^2(I_{md}) + u^2(I_{mconv})}$$

The terms relative to air buoyancy (mb) and convection effects (mconv) are considered negligible due to enough acclimatisation allowed to the instrument.

Expanded uncertainty has been computed with the following formula:

$$U = u(E)_{max} k$$

For this report a coverage factor of 2 as been considered giving an overall confidence level of 95,45%