

|                |                 |               |            |
|----------------|-----------------|---------------|------------|
| Certificate N° | 000004/2021     | Date of issue | 31.03.21   |
| Client         | ENEL Produzione | Work order    | 8000000591 |

## Instrument specification

|                  |                         |              |                |                  |                 |
|------------------|-------------------------|--------------|----------------|------------------|-----------------|
| Type             | Turbidity meter         | Manufacturer | Endress-Hauser | Serial number    | E3087305G00     |
| Min capacity     | 0                       | Max capacity | 80             | Model            | Liquiline CM442 |
| Readability At 0 | 0,1                     | Readability  | 0,1            | Unit of measure  | FNU             |
| Description      | C1 Itar Turbidity meter |              |                | Next Calibration | 30.06.21        |

## Test ambient conditions

|             |                |          |     |              |          |       |
|-------------|----------------|----------|-----|--------------|----------|-------|
| Location    | ENEL - C1 Itar |          |     | Date of test | 31.03.21 | 00:00 |
| Temperature | 23,5°C         | Humidity | 72% | Pressure     | 1020hPa  |       |

## Standard certificates used

| Name      | Number | Issuer | Date of issue |
|-----------|--------|--------|---------------|
| Turbidity | 852    | DPG    | 24.05.19      |

## Calibration summary

| Test          | Certificate name | Uncertainty | Temperature | Humidity | Pressure |
|---------------|------------------|-------------|-------------|----------|----------|
| Repeatability | Turbidity        | 0,707696FNU | 23,0°C      | 71%      | 1021hPa  |
| Linearity     | Turbidity        | 0,719954FNU | 23°C        | 70%      | 1021hPa  |

Expanded uncertainty **1,439907FNU**

## Notes


*Provenza*  
Technician  
Dipietro Group S.r.l.  
P. Pavesi, 2 - V.le Garrone, 6  
96010 Città Giardino - Melilli (SI)  
P. IVA 01142700891

Instrument

Turbidity meter - Liquiline CM442 - E3087305G00

| Repeatability |               |                    |            |           | Standard reference |             |      |
|---------------|---------------|--------------------|------------|-----------|--------------------|-------------|------|
| Measure       | Nominal value | Conventional value | Read value | Deviation | Serial             | Uncertainty | OIML |
| 1             | 15            | 14,95              | 15         | 0,05      | HI9873-20          | 0,1         |      |
| 2             | 15            | 14,95              | 15         | 0,05      | HI9873-20          | 0,1         |      |
| 3             | 15            | 14,95              | 14         | -0,95     | HI9873-20          | 0,1         |      |
| 4             | 15            | 14,95              | 15         | 0,05      | HI9873-20          | 0,1         |      |
| 5             | 15            | 14,95              | 16         | 1,05      | HI9873-20          | 0,1         |      |

Min value 14 Max value 16 Average value 15  
Standard deviation ( $\sigma$ ) 0,707107 Repeatability uncertainty 0,707696

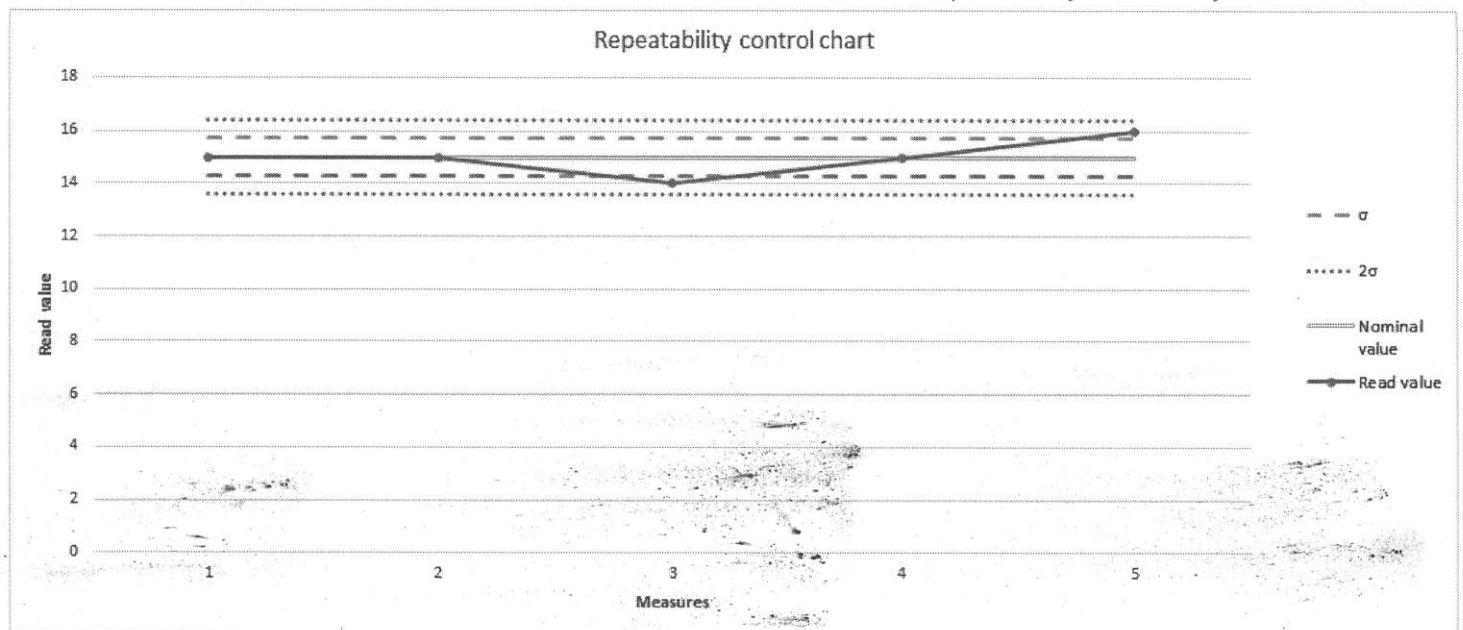

Dipietro Group S.r.l.  
Technician  
Il Traversa a V.le Garrone,6  
96019 Provenga (SR)  
P. IVA 01112700891




Instrument

Turbidity meter - Liquiline CM442 - E3087305G00

| Linearity |               |                    |            |       |  | Uncertainty of error | Standard reference |
|-----------|---------------|--------------------|------------|-------|--|----------------------|--------------------|
| Measure   | Nominal value | Conventional value | Read value | Error |  |                      | Uncertainty OIML   |
| 1         | 15            | 14,95              | 14         | -0,95 |  | 0,719954             | 0,1                |

Min value 14 Max value 14 Average value 14

Standard deviation 0,95 k-Factor: 2 (95,45%) Expanded uncertainty 1,439907

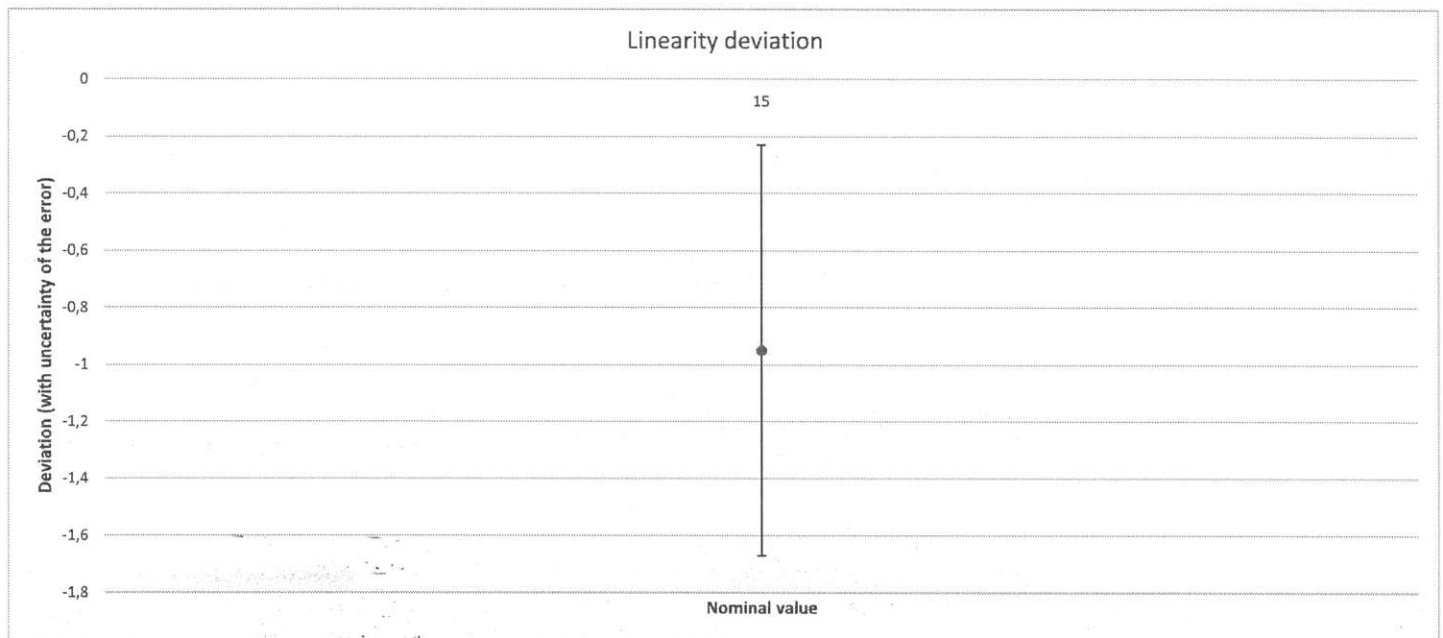

Di Pietro Group S.r.l.  
 Il Traversa a V.le Garrone, 6  
 96019 Citta' Giardino - Melilli (SR)  
 P. IVA 01112700891

## Formulas

### Repeatability

The test consists in the repeated measure of the same reference value, under identical conditions of handling the reference and the instrument, and under constant test conditions, both as far as possible

Standard deviation is computed to allow an appraisal of the instrument's performance.

$$s(I) = \sqrt{\frac{1}{n-1} \sum_{i=1}^n (I_i - \bar{I})^2} \quad \bar{I} = \frac{1}{n} \sum_{i=1}^n I_i$$

Repeatability standard uncertainty has been computed with the following formula, taking into account instrument's scale interval (d)

$$u_{rep} = \sqrt{s(I)^2 + \left(\frac{d_I^2}{12}\right)}$$

### Linearity

This test is performed with different test values distributed fairly evenly over the normal measuring range. The purpose of this test is an appraisal of the performance of the instrument over the whole measuring range.

The uncertainty of the error is computed with the following formula and takes into account repeatability and eccentricity uncertainty when applicable:

$$u(E) = \sqrt{u^2(I_{dig0}) + u^2(I_{dig1}) + u^2(I_{rep}) + u^2(I_{ecc}) + u^2(I_{mc}) + u^2(I_{mb}) + u^2(I_{md}) + u^2(I_{mconv})}$$

The terms relative to air buoyancy (mb) and convection effects (mconv) are considered negligible due to enough acclimatisation allowed to the instrument.

Expanded uncertainty has been computed with the following formula:

$$U = u(E)_{max} k$$

For this report a coverage factor of 2 as been considered giving an overall confidence level of 95,45%